

Keysight Technologies

PNA Microwave Network Analyzers

Introduction to Application Development

Application Note

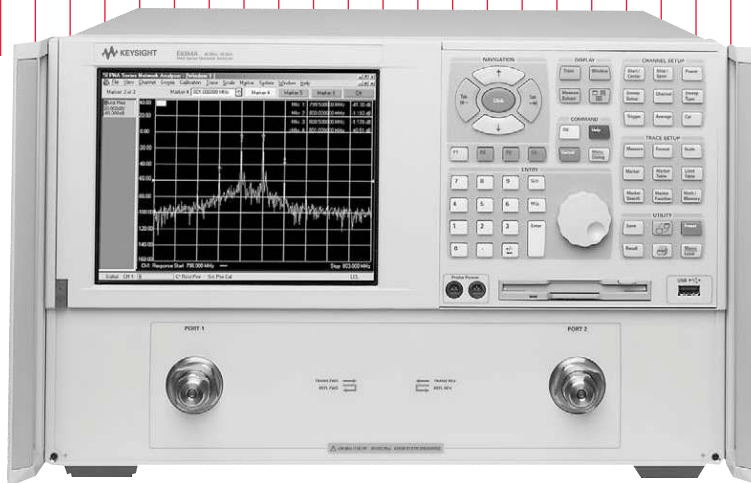


Table of Contents

| | |
|--|----|
| Introduction | 4 |
| How to Use this Document | 4 |
| Basic Administration | 5 |
| Registering as a User on the PNA | 5 |
| Sharing Drives Between the PNA and a PC | 7 |
| Determine the Full Computer Names of Both Devices | 7 |
| Share the PNA's C Drive | 8 |
| Map a New Drive on the PC | 8 |
| Installing Software | 9 |
| Installing Software Over the LAN | 9 |
| Map the PC's CD-ROM Drive to the PNA | 9 |
| Install the Software | 9 |
| Installing Software from External USB CD-ROM Drive | 10 |
| Connect the External CD Drive to the PNA | 10 |
| Install the Software | 10 |
| Configuring COM/DCOM | 11 |
| Workgroups versus Domains | 11 |
| Granting Access to a Specific User | 12 |
| Windows XP Procedure for Granting Access | 12 |
| Windows 2000 Procedure for Granting Access | 12 |
| Configuring the PC for DCOM Access | 13 |
| If You Encounter Problems | 13 |
| Application Examples | 14 |
| Microsoft Visual Basic Example | 15 |
| Visual Basic Configuration | 15 |
| Visual Basic Code | 16 |
| Visual Basic Output | 17 |
| Microsoft Visual Basic Script (VBScript) Example | 18 |
| VBScript Configuration | 18 |
| VBScript Code | 18 |
| VB Script Output | 19 |
| Microsoft Word Example | 20 |
| Microsoft Word Configuration | 20 |
| Microsoft Word Code | 21 |
| Microsoft Word Output | 22 |
| Microsoft Excel Example | 23 |
| Microsoft Excel Configuration | 23 |
| Microsoft Excel Code | 24 |
| Microsoft Excel Output | 25 |
| Microsoft Visual C++ Example | 26 |
| Microsoft Visual C++ Configuration | 26 |
| Microsoft Visual C++ Code | 26 |
| Microsoft Visual C++ Output | 28 |
| Keysight VEE Example | 29 |
| Keysight VEE Configuration | 29 |
| Keysight Vee Code | 30 |
| Keysight Vee Output | 31 |
| National Instruments LabVIEW™ Example | 32 |
| LabVIEW Configuration | 32 |
| LabVIEW Code | 32 |
| LabVIEW Output | 32 |

| | |
|---|-----|
| Appendix A: Quick Reference Guide | .33 |
| Register a User on the PNA | .33 |
| Share Drives | .33 |
| Configure COM/DCOM | .34 |
| Grant User Access (Windows XP) | .34 |
| Grant User Access (Windows 2000) | .34 |
| Configure the PC for DCOM Access | .34 |
| Appendix B: PNA and PNA-L Models | .35 |
| Web Resources | .35 |

Introduction

This application note provides a step-by-step guide to system administration, software installation, and COM/DCOM¹ setup for the PNA Series² of microwave network analyzers. After reading this application note, you should be able to:

- Add user profiles to your analyzer
- Share drives between your analyzer and a PC running Windows
- Load software on your analyzer over the LAN or from an external CD drive
- Configure your analyzer and PC for COM/DCOM communications

Additionally, this application note provides a simple programming example in six common languages or formats³ (Microsoft Visual Basic, Visual Basic Script, Word, Excel, Keysight VEE, Visual C++, and National Instruments LabVIEW) that demonstrates the differences between development platforms.

The procedures listed in this application note are valid for a PC with Windows 98 or newer operating systems. This application note was developed on a PC with Windows 2000 Professional version 5.00.2195 with service pack 4. The PNA's operating system was Windows 2000 Professional, however, the steps should be similar for other versions of Windows operating systems.

How to Use This Document

Depending upon what you are trying to accomplish, you may not need to perform all of the steps and procedures set forth in this document. Use the following as guideline.

If you want to:

- **Add a user so that they can log into the PNA or use the PNA via DCOM**, perform "Registering as a User on the PNA" on page 5.
- **Transfer files between the PNA and a PC**, perform "Sharing Drives Between the PNA and a PC" on page 7. You may also want to add other users. If so, see "Registering as a User on the PNA" on page 5.
- **Installing software on the PNA**, see "Error! Reference source not found." on page 9 **Error! Bookmark not defined...**
- **Run a program on the PC that accesses the PNA via DCOM**, perform "Registering as a User on the PNA" on page 5, and "Configuring COM/DCOM" on page 11. "Installing Software" on page 9 may also be of interest.

1. COM = component object model, DCOM = distributed component object model
2. "PNA" or just "analyzer" will be used throughout this document to refer to both PNA and PNA-L network analyzers.
3. Microsoft Word and Excel use Visual Basic for Applications

Basic Administration

This section describes how to add a user on the PNA and how to share drives between the analyzer and a PC.

To obtain access to the PNA for COM/DCOM, a user must be registered on the analyzer.

Any drive can be shared between the analyzer and PC, including a CD drive for software installation over the LAN (described in further detail in “Installing Software Over the LAN” on page 9). To configure COM/DCOM communications to and from the PC and analyzer, share the analyzer’s (C:) drive with your PC.

Registering as a User on the PNA

When accessing the PNA from a PC using DCOM, the user must be registered on the PNA using the same name and password as that used on the PC, or the user must follow a special procedure to allow access. That special procedure is not documented here, but can be found at <http://na.tm.keysight.com/pna/DCOMSecurity.html>.

To register with the user’s PC login and password, refer to the following procedure. The following tasks must be performed by an administrator of the PNA.

On the PNA:


1. Log on to the PNA using the administrator user name and password.
2. Right-click on the **My Computer** icon, and then click on **Manage** to launch the Computer Management utility.
3. In the Computer Management window, expand **Local Users and Groups** and then click on **Users** to view the current list of users in the right side of the window.
4. Launch the New User window by right-clicking on the **Users** folder and then clicking on **New User**. See screenshot, below.

Note

This is the same procedure a system administrator must use to grant multiple users permission to log on to the analyzer and maintain their user profile.

Note

When the analyzer is shipped from the factory, the default administrator name is **PNA-Admin**, and the default password is **keysight**. This is true of all PNAs shipped after April, 2004. Earlier units had the administrator name of **administrator** and either a blank password, or the password **tsunami**.

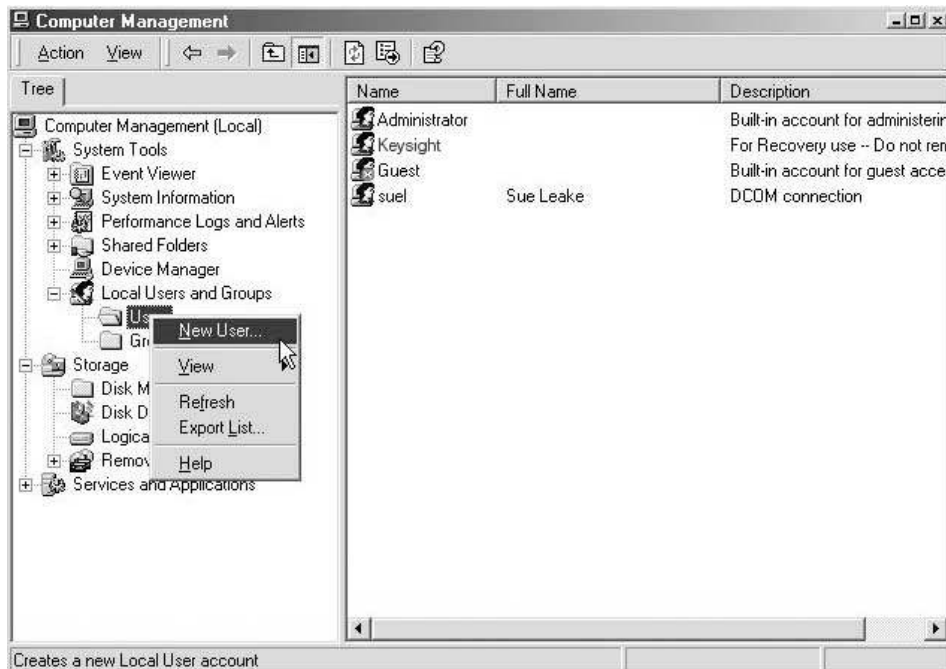

Basic Administration (continued)

5. Enter the user's PC login into the **User name** field. Enter the user's PC password into the **Password** and **Confirm password** fields. Click **Create** when done entering information.

Optional fields

Recommended

Note

The **Full name** and **Description** fields are optional. The **User must change password at next logon** box is the default. In most cases it is recommended that you select **Password never expires**.

6. The **New User** window will not close, but the input boxes are cleared and the check boxes returned to their default settings. Click the **Close** button to **close** the **New User** window. Notice that the new user has been added to the list in the **Computer Management** window. Close the **Computer Management** window. The user now has access to the PNA.

Sharing Drives Between the PNA and a PC


Any drive can be shared between the analyzer and a PC, including a CD drive for software installation over the LAN. This section contains the steps necessary to share drives between your computer and the analyzer, and specifically shows how to share the (C:) hard drives. These steps may be useful for configuring COM/DCOM access (see page 11).

Both the PC and the PNA must be connected to the same LAN before continuing.

Determine the Full Computer Names of Both Devices

Perform the following steps on both the PC and the PNA:

1. Right-click the **My Computer** icon, and then click **Properties**.
2. Click the **Network Identification** or **Computer Name** tab to view the **Full computer name** for the device.
3. Record the computer names here:

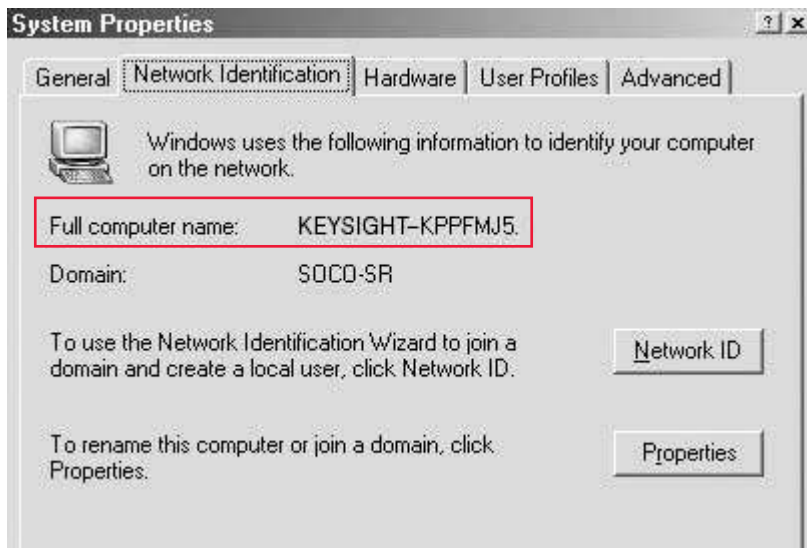

PC name: _____

PNA name: _____

Note

The following sections describe how to access the PNA's (C:) drive from your PC. You can access your PC's (C:) drive from the analyzer by simply performing the PNA steps on the PC, and vice versa.

Share the PNA's (C:) Drive


On the PNA:

1. Double-click **My Computer**, right-click on **Local Disk (C:)**, and then select **Sharing...**
2. Ensure that **Share this folder** is selected. If you choose to use a different **Share name** than the default of **C\$**, enter it in the **Share name** field and make note of it for future reference.
3. Click **OK** when done.

Map a New Drive on the PC

On the PC:

1. Right-click on **My Computer** and select **Map Network Drive**.
2. The Map Network Drive wizard will select an available drive letter for you. You may also use any other available drive letter. Record the drive letter here: _____.
3. Enter the path to the PNA in the Folder field. The syntax is "\\computername\share name". See the example below.

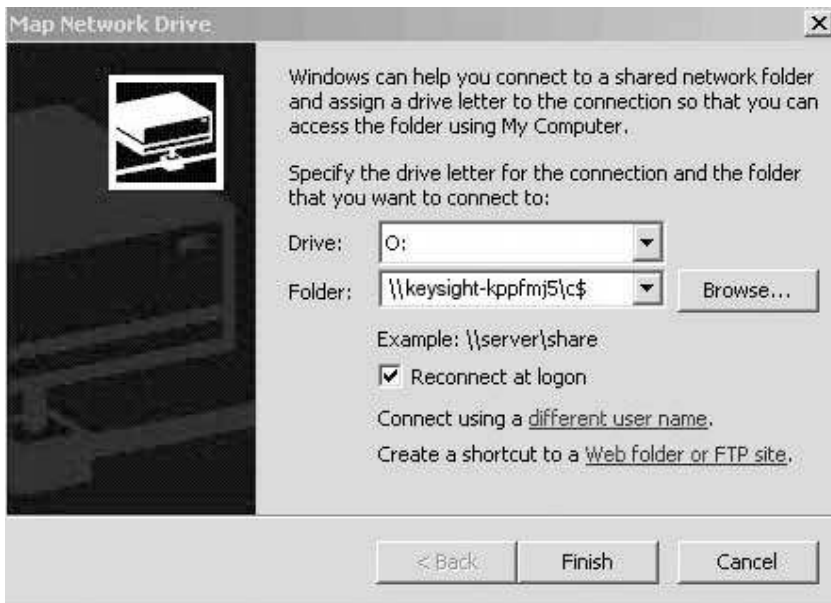

4. If you want your PC to automatically map this drive every time you log on to your PC, select **Reconnect at logon**.
5. Click **Finish**. (If the user name/password is not identical on both the PC and the PNA, Windows will first ask for a valid name and password.) Verify that the drive is visible in the **My Computer** folder on your PC.

Installing Software

This section assumes that you will be installing software from a CD-ROM. You can either use your PC's CD-ROM drive, or a USB external CD-ROM drive connected to the PNA.

If you will be using the CD-ROM drive on your PC to install the software on the analyzer, go to "Installing Software Over the LAN" below. Otherwise, if you will be using an external USB CD-ROM drive connected to the PNA, go to "Installing Software from External USB CD-ROM Drive" on page 10.

Installing Software Over the LAN

If you do not have access to a USB external CD-ROM drive for your PNA, it is possible to map your PC's CD-ROM drive to the PNA. Both your PC and the analyzer must be connected to the LAN. The software can then be installed from your PC's CD drive.

Map the PC's CD-ROM Drive to the PNA

On the PC:

1. Double-click **My Computer**. Right-click on the icon that represents the CD-ROM drive, and select **Properties**.
2. Select the **Sharing** tab and record the **Share name** of the CD-ROM drive here:
_____.
3. Obtain your PC's full computer name. See "Determine the Full Computer Names of Both Devices" on page 7.

On the PNA:

4. Map a drive from the PNA to the PC's CD-ROM drive. See steps 1 through 5 on page 8 for general instructions. Be sure to perform these steps on the PNA and to use the computer name of the PC along with the share name obtained in step 2, above.

Install the Software

5. Insert the software CD into your PC's CD-ROM drive.
6. On the PNA, double-click **My Computer** and then double-click the icon representing the new drive that was mapped in step 4.
7. Refer to your software's documentation to determine which file to run for setup and installation. Be sure to choose the PNA's (C:) drive as the destination for file installation.

Note

If your user settings (see step 5 on page 6) were set to something other than your PC login and password, you will need to "Connect using different user name."

Installing Software from External USB CD-ROM Drive

This procedure was verified for an Iomega Predator CD-RW drive. Perform all steps in this procedure on the PNA. If your PNA already has an external USB CD drive connected, skip to step 5.

Connect the External CD Drive to the PNA

1. Exit all applications, including the network analyzer application.
2. Connect the external CD drive to an available USB port on the analyzer or to a USB hub that is connected to the analyzer.
3. If applicable, connect the power cord for the CD drive to an available outlet. If the drive has an on/off switch, switch the CD drive to On.
4. The Windows system in the PNA should automatically recognize and install the new CD drive. Follow any instructions for installing drivers and/or rebooting the system. (If you are using the CD drive for *reading* files only (no writing), then drivers should not be necessary.)

Install the Software

5. Insert the software CD into the external CD drive.
6. Most software CDs are designed to start automatically. If the setup application for your software does not start, refer to the software documentation to determine which file to run for setup and installation.

Configuring COM/DCOM

This section briefly describes the concepts of workgroups and domains. It then explains the steps necessary to grant DCOM access to a specific user, and finally describes how to configure the user's PC for DCOM access.

Workgroups versus Domains

Before continuing you may need to consider the differences between setting up the PNA as a member of a workgroup or a domain.

- A **workgroup** is established and maintained by the PNA administrator. The PNA is shipped from the factory configured as a member of a workgroup named WORKGROUP. Also by default from the factory, **Everyone** (all members of WORKGROUP) has permission to launch and access the PNA application via COM/DCOM.
- A **domain** is typically a large organizational group of computers. A network administrator must establish and maintain the domain and control which devices have membership in the domain.

This document assumes that the analyzer will remain a member of a workgroup. It also assumes that the PNA administrator will want to give specific users (not **Everyone**) COM/DCOM permissions.

Note

The information provided here is also available in more detail in the PNA's Help software titled "Configure for COM-DCOM Programming." If you encounter trouble performing the procedures in this section, please refer to the online help; (available on the web) at: <http://www.keysight.com/find/pna> > **Specify product page**, such as 88364B, > Library > Manuals & Guide > Online Help, the online help will always have the most up-to-date version of the procedures in this section.

Note

If your DCOM program will be using events, and your PC is on a domain, it is best to put your PNA into the same domain. The use of events typically requires a "trust relationship" between the client and server; putting the PNA into the same domain will satisfy this requirement.

Granting Access to a Specific User

You may not need to perform this procedure. Read the following note to determine whether or not you want to do this.

Select the appropriate procedure below depending on your operating system.

Windows XP Procedure for Granting Access

Minimize the PNA application before beginning. All steps in this procedure are performed on the PNA.

1. Click the Windows **Start** button, then select **Run**. Enter “**dcomcnfg**” into the text box and click **OK**.
2. Open the following folder sequence:
Component Services Window
Component Services
Computers
My Computer
DCOM Config
3. Right-click on **Keysight PNA Series**, then click **Properties**.
4. Select the **Security** tab and click **Customize** under **Access Permissions**, and then click the **Edit...** button.
5. Select **Everyone**, then click **Remove**.
6. Click **Add** and type a group name or user account name to add. Click **OK**.
7. Under **Launch Permissions**, click **Customize**, then click **Edit**.
8. Select **Everyone**, then click **Remove**.
9. Click **Add** and type a group name or user account name to add. Click **OK**.

Note

The analyzer is shipped from the factory granting access to “Everyone.” Everyone is defined as only those users who have been given logon accounts on the PNA. Use the following procedure only if you want to prevent Everyone from having DCOM access to the PNA, and to allow DCOM access only to those individuals that you specify.

Windows 2000 Procedure for Granting Access

Minimize the PNA application before beginning. All steps in this procedure are performed on the PNA.

1. Click the Windows Start button, then select **Run**. Enter “**dcomcnfg**” into the text box and click **OK**. The **Distributed COM Configuration Properties** window should appear.
2. Make sure the **Applications** tab is on top, select **Keysight PNA Series**, and then click the **Properties...** button.
3. Select the **Security** tab, click **Use custom access permissions**, and then click the **Edit...** button.
4. In **Registry Value Permission**, select **Everyone**, then click **Remove**.
5. Click **Add** and then select one or more groups, or specific users. To give specific users access, click **Show Users** or **Members**, then select the name from the list.
6. Click **Add**, then click **OK**.
7. Click **Use custom launch permissions**, then click **Edit**.
8. In **Registry Value Permissions**, select **Everyone**, then click **Remove**.
9. Click **Add**, and then select one or more groups, or specific users. To give specific users launch permission, click **Show Users** or **Members**, then select the name from the list.
10. Click **Add**, then click **OK**.

Configuring the PC for DCOM Access

On your PC, there is a registry file that keeps track of where object models are located. Therefore, you must register the type library on the PC that will be used to develop code and run the program. A program called **pnaproxy.exe** will perform all the necessary tasks. This program is located on the PNA's hard drive in the following location:

C:\Program Files\Keysight\Network Analyzer\Automation

Copy the pnaproxy.exe program (approximately 5 MB) to any convenient location on your PC. You can use a USB pen drive, or you can map a drive to the PNA from your PC and copy it over the LAN. See "Map a New Drive on the PC" on page 8.

Note

To register the type library on your PC, you must be logged on as an administrator of your PC.

The procedure below will accomplish the following:

- Register the network analyzer application on your PC
 - Copy and register the proxystub (835xps.dll) onto your PC
 - Copy and register the PNA type library (835x.tlb) onto your PC
 - Copy and register the FCA¹ type library (fca.tlb) onto your PC
1. Close any applications that are currently running on your PC.
 2. Navigate to, and double-click the **pnaproxy.exe** file that you copied to your PC.
 3. Follow the instructions to install PNA proxy. (If the installation offers a choice, of Modify, Repair, or Remove, select **Remove**. Then double-click on **pnaproxy.exe** again when it has finished.)
 4. When prompted, type the computer name of the PNA that you want to use as the default target. See "Determine the Full Computer Names of Both Devices" on page 7 for information on determining the name of the PNA. Alternately, you can provide a fixed IP address instead of a name.
 5. When the installation is complete, the PNA and FCA type libraries should be registered on your PC.
 6. Your programming environment may require you to set a reference to the PNA type library that is now located on your PC. For example, in Visual Basic, click **Project > References**. Then browse to **C:\Program Files\Common Files\Keysight\PNA** and select **835x.tlb**.

If You Encounter Problems

- Be sure that you do not have any applications running on the PC.
- Check that both the account name and password used on both the PNA and PC match *exactly*.
- Repeat the procedure outlined in "Configuring the PC for DCOM Access" above.
- If you still get errors, see <http://na.tm.keysight.com/pna/DCOMSecurity.html>.

1. FCA = frequency converter application

Application Examples

The analyzer's support for DCOM over the LAN provides control of the PNA using a variety of platforms. DCOM acts as an interface to the analyzer for external applications. With DCOM, the programmer can develop an application on an external computer. During development, the application will interface to the analyzer over the LAN through the DCOM interface. Once the developer has finished the application, it can be distributed to the analyzer. After it has been distributed to the analyzer, the application will interface with the PNA using COM.

The example applications in this application note were developed in a number of different programming languages to show the differences between development platforms. The application was first developed on a PC and then transferred to the analyzer once development was complete. The table below outlines the setup parameters that the applications will use to configure the PNA analyzer for a measurement:

| Parameter | Value |
|-------------------|------------------------|
| Start frequency | 1 GHz |
| Stop frequency | 2 GHz |
| Number of points | 11 |
| Measurement | S_{11} |
| Data storage area | Uncorrected (Raw Data) |
| Data format | Log Magnitude |
| Trigger mode | Single |

The device tested was a 50 ohm standard load on port 1 of the PNA.


You can download the example programs and obtain more detailed information for each development environment from <http://na.tm.keysight.com/pna>

The development environment should reference the type library associated with the PNA. For example, in Visual Basic, add the "Keysight PNA Series 1.9 Type library" as a reference. This will allow the program to "see" the various classes and methods available for use with the analyzer during development. (See the individual programming examples that follow for more information.)


Microsoft Visual Basic Example

Visual Basic Configuration

The type library for the PNA should be referenced in the Visual Basic development environment. The following figure has the type library for the PNA highlighted.

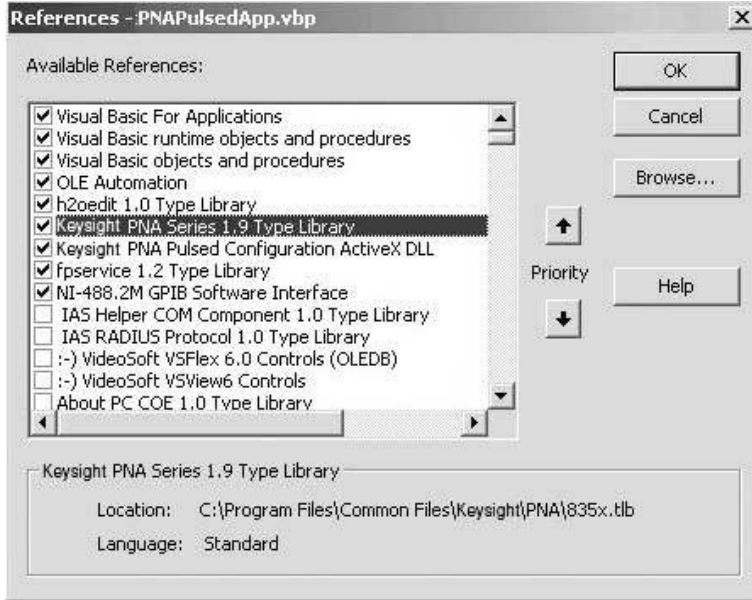

Using the Visual Basic Object Browser the developer can see what classes and methods are available for development of applications for the analyzer (see figure below).

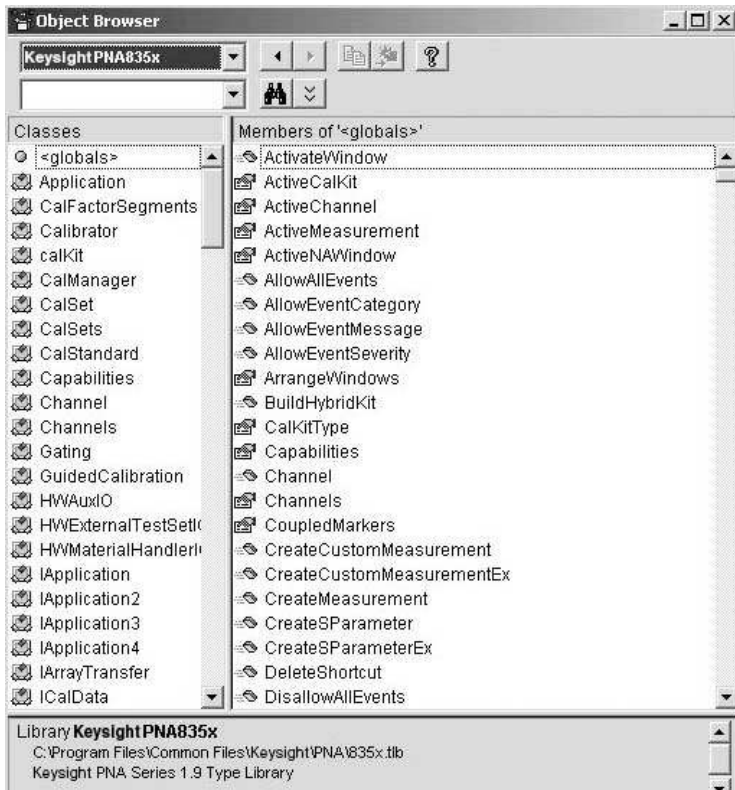

Visual Basic Code

The application code is contained below. To run the application, first generate the executable file. Once this is complete, it can be copied and executed on the analyzer or run on the PC. The application can also be run from the development environment.

Note


Be sure to edit the first line of code in Sub Main to include the name of your analyzer.

```
Option Explicit
Dim app As KeysightPNA835x.Application
Dim chan As KeysightPNA835x.Channel
Dim meas As KeysightPNA835x.Measurement
Dim result As Variant
Dim i As Integer
Dim num_points As Integer
Dim message As String

Private Sub Main()
    'Connect to the PNA application on machine SLTSU044
    Set app = CreateObject("KeysightPNA835x.Application","SLTSU044")
    'Reset the analyzer to instrument preset
    app.Reset
    'Create S11 measurement
    app.CreateMeasurement 1, "S11", 1
    'Set chan variable to point to the active channel
    Set chan = app.ActiveChannel
    'Set meas variable to point to the active measurement
    Set meas = app.ActiveMeasurement
    'Setup the channel for a single trigger
    chan.Hold True
    app.TriggerSignal = naTriggerManual
    chan.TriggerMode = naTriggerModeMeasurement
    'Make the PNA application visible
    app.Visible = True
    'Set channel parameters
    chan.NumberOfPoints = 11
    chan.StartFrequency = (1000000000#)
    chan.StopFrequency = (2000000000#)
    'Send a manual trigger to initiate a single sweep
    chan.Single True
    'Store the data in the "result" variable
    result = meas.GetData(naRawData, naDataFormat_LogMag)
    'Display the result
    num_points = chan.NumberOfPoints
    For i = 0 To num_points - 1
        message = message & result(i) & vbCrLf
    Next
    If MsgBox(message, vbOKOnly, "S11(dB) - VBS COM
    Example for PNA") Then
        Set chan = Nothing
        Set app = Nothing
    End If
End Sub
```

Visual Basic Output

The figure below shows the displayed results when the application is executed.

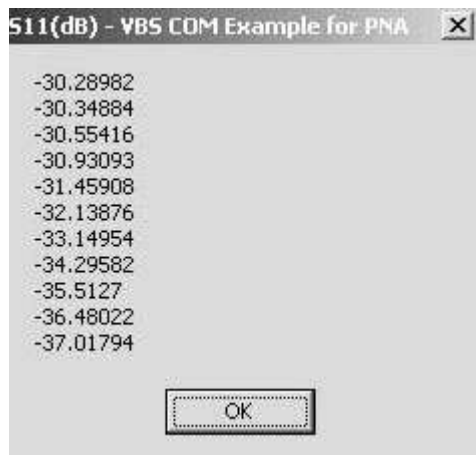

Microsoft Visual Basic Script (VBScript) Example

VBScript Configuration

Some operating systems may require that the Visual Basic Scripting engine be installed before running the application on a PC. To download a free copy of a Visual Basic Scripting engine, visit the following web site: <http://msdn.microsoft.com/scripting/>

VBScript Code

The application code is contained below. The developer must save the file in a text file (i.e. using notepad) and save it with the “.vbs” extension. The “.vbs” extension will tell the operating system to execute the code using the Visual Basic Scripting engine. In order to run the application, double-click on the saved .vbs file. The application can be run on a PC or copied and run on the PNA.


```
Option Explicit
'Shell objects
Dim app
Dim chan
Dim meas
Dim result
Dim message
Dim num_points
Dim I
'Connect to the PNA application on machine SLTSU044
Set app = CreateObject("KeysightPNA835x.Application","SLTSU044")
'Reset the analyzer to instrument preset
app.Reset
'Create S11 measurement
app.CreateMeasurement 1, "S11", 1
'Set chan variable to point to the active channel
Set chan = app.ActiveChannel
'Set meas variable to point to the active measurement
Set meas = app.ActiveMeasurement
'Setup the channel for a single trigger
chan.Hold True
app.TriggerSignal = 3
chan.TriggerMode = 1
'Make the PNA application visible
app.Visible = True
'Set channel parameters
chan.NumberOfPoints = 11
chan.StartFrequency = (1000000000)
chan.StopFrequency = (2000000000)
'Send a manual trigger to initiate a single sweep
chan.Single True
'Store the data in the "result" variable
result = meas.GetData(0, 1)
'Display the result
num_points = chan.NumberOfPoints
For i = 0 To num_points - 1
    message = message & result(i) & vbCRLF
Next
if MsgBox(message, vbOKOnly, "S11(dB) - VBS COM
Example for PNA") then
    Set chan = Nothing
    Set app = Nothing
end if
```

Note

Be sure to edit the “Set app = Create-Object...” code to include the name of your analyzer.

VB Script Output

The figure below shows the displayed results when the application is executed.

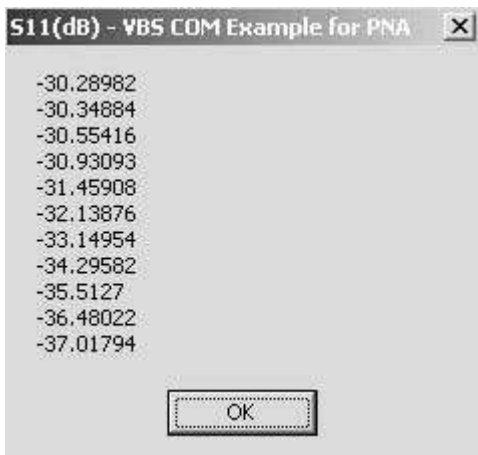

Microsoft Word Example


Microsoft Word Configuration

Microsoft Office 2000 was used for this example. This version of Office contains Visual Basic for Applications (VBA) which allows developers to attach Visual Basic Macros to Word documents. To run this example:

1. Create a new Word document with a table that has 2 columns and 12 rows as shown below. Enter the headings into the first row, and the frequency values in the first column.

| Frequency in MHz | S ₁₁ in dB |
|------------------|-----------------------|
| 1.0 | |
| 1.1 | |
| 1.2 | |
| 1.3 | |
| 1.4 | |
| 1.5 | |
| 1.6 | |
| 1.7 | |
| 1.8 | |
| 1.9 | |
| 2.0 | |

2. In the Word application, select **Tools > Macro > Visual Basic Editor**.
3. Double-click **ThisDocument** in the Visual Basic Editor Project window.
4. Copy the code from Microsoft Word Code on page 21 into the Visual Basic Editor window.

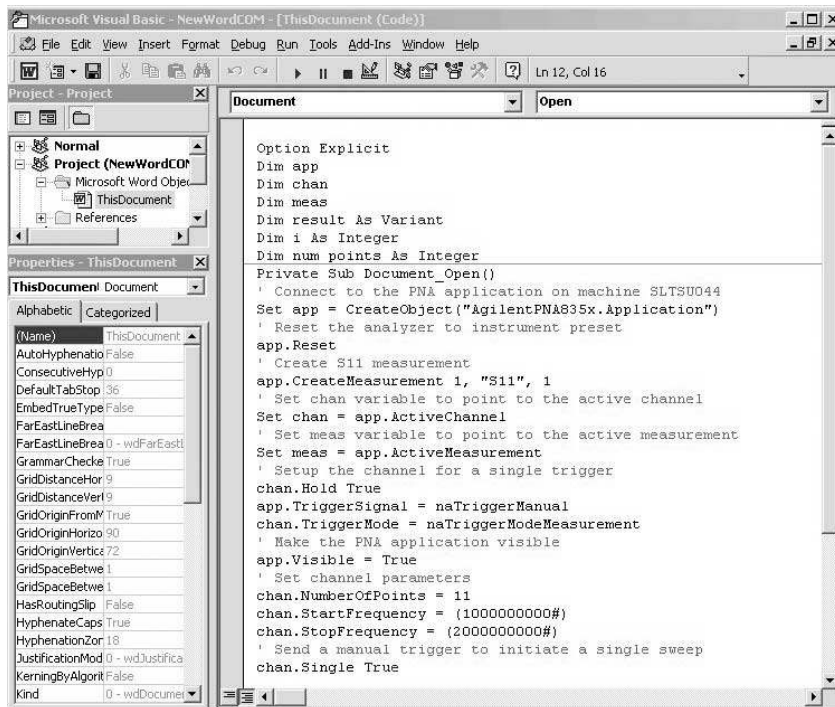

5. The type library for the PNA should be referenced in the Visual Basic development environment. (Select **Tools > References** in the Visual Basic Editor, and be sure to select the Keysight PNA Series Type Library.) See the screenshot on page 15 for an example of the References window.
6. Save and close the file.

Note

In this example the "CreateObject" method will look at the configuration of DCOM to see what machine to connect to.

Microsoft Word Code

The application code is contained below. The program inserts the data retrieved from the analyzer into an existing table in a Word document. To run the application, open the document using Microsoft Word. Enable the macros when prompted. Once this is complete, the application will execute and update the document. The application can be run on a PC or the analyzer.

Note

Be sure to edit the first line of code in Sub Document_Open to include the name of your analyzer.

```
Option Explicit
Dim app
Dim chan
Dim meas
Dim result As Variant
Dim i As Integer
Dim num_points As Integer
Private Sub Document_Open()
    'Connect to the PNA application on machine SLTSU044
    Set app =
CreateObject("KeysightPNA835x.Application","SLTSU044")
    'Reset the analyzer to instrument preset
    app.Reset
    'Create S11 measurement
    app.CreateMeasurement 1, "S11", 1
    'Set chan variable to point to the active channel
    Set chan = app.ActiveChannel
    'Set meas variable to point to the active measurement
    Set meas = app.ActiveMeasurement
    'Setup the channel for a single trigger
    chan.Hold True
    app.TriggerSignal = naTriggerManual
    chan.TriggerMode = naTriggerModeMeasurement
    'Make the PNA application visible
    app.Visible = True
    'Set channel parameters
    chan.NumberOfPoints = 11
    chan.StartFrequency = (1000000000#)
    chan.StopFrequency = (2000000000#)
    'Send a manual trigger to initiate a single sweep
    chan.Single True
    'Store the data in the "result" variable
    result = meas.GetData(naRawData,naDataFormat_LogMag)
    'Display the result
    num_points = chan.NumberOfPoints
    For i = 0 To num_points - 1
        ThisDocument.Tables(1).Cell(i + 2, 2).Range = result(i)
    Next
    Set chan = Nothing
    Set app = Nothing
End Sub
```

Microsoft Word Output

The figure below shows the displayed results when the application is executed.

| Frequency in MHz | S₁₁ in dB |
|-------------------------|-----------------------------|
| 1.0 | -30.69699 |
| 1.1 | -30.66298 |
| 1.2 | -30.8582 |
| 1.3 | -31.1689 |
| 1.4 | -31.64268 |
| 1.5 | -32.23172 |
| 1.6 | -33.18055 |
| 1.7 | -34.23394 |
| 1.8 | -35.35485 |
| 1.9 | -36.38187 |
| 2.0 | -37.03015 |

Microsoft Excel Example

Microsoft Excel Configuration

Microsoft Office 2000 was used for this example. This version of Office contains Visual Basic for Applications (VBA) which allows developers to attach Visual Basic Macros to Excel documents. To run this example:

1. Create and format a new Excel document with appropriate text headings and graphs if desired. The program will insert S_{11} values in column A, cells 3 through 13.
2. In the Excel application, select **Tools > Macro > Visual Basic Editor**.
3. Double-click **ThisWorkbook** in the Visual Basic Editor Project window. Copy the code from Microsoft Excel Code on page 24 into the Visual Basic Editor window.
4. The type library for the PNA should be referenced in the Visual Basic development environment. (Select **Tools > References** in the Visual Basic Editor, and be sure to select the Keysight PNA Series Type Library.) See the screenshot on page 15 for an example of the References window.
5. Save and close the Excel file.

Microsoft Excel Code

The application code is contained below. The program inserts the data retrieved from the analyzer into cells A3 through A13 in the Excel document. To run the application, open the document using Microsoft Excel. Enable the macros when prompted. Once this is complete, the application will execute and update the document. You can then create a graph (as shown in the example on page 32). The data and graph will then update with each subsequent run of the application. The application can be run on a PC or the analyzer.

Note

Be sure to edit the first line of code in Sub Workbook_Open to include the name of your analyzer.

```


Option Explicit
Dim app
Dim chan
Dim meas
Dim result As Variant
Dim i As Integer
Dim num_points As Integer

Private Sub Workbook_Open()
    'Connect to the PNA application on machine SLTSU044
    Set app =
    CreateObject("KeysightPNA835x.Application","SLTSU044")
    'Reset the analyzer to instrument preset
    app.Reset
    'Create S11 measurement
    app.CreateMeasurement 1, "S11", 1
    'Set chan variable to point to the active channel
    Set chan = app.ActiveChannel
    'Set meas variable to point to the active measurement
    Set meas = app.ActiveMeasurement
    'Setup the channel for a single trigger
    chan.Hold True
    app.TriggerSignal = naTriggerManual
    chan.TriggerMode = naTriggerModeMeasurement
    'Make the PNA application visible
    app.Visible = True
    'Set channel parameters
    chan.NumberOfPoints = 11
    chan.StartFrequency = (1000000000#)
    chan.StopFrequency = (2000000000#)
    'Send a manual trigger to initiate a single sweep
    chan.Single True
    'Store the data in the "result" variable
    result = meas.GetData(naRawData, naDataFormat_LogMag)
    'Display the result
    num_points = chan.NumberOfPoints
    For i = 0 To num_points - 1
        Sheet1.Cells(3 + i, 1) = result(i)
    Next
    Set chan = Nothing
    Set app = Nothing
End Sub

```

Microsoft Excel Output

The figure below shows the displayed results when the application is executed.

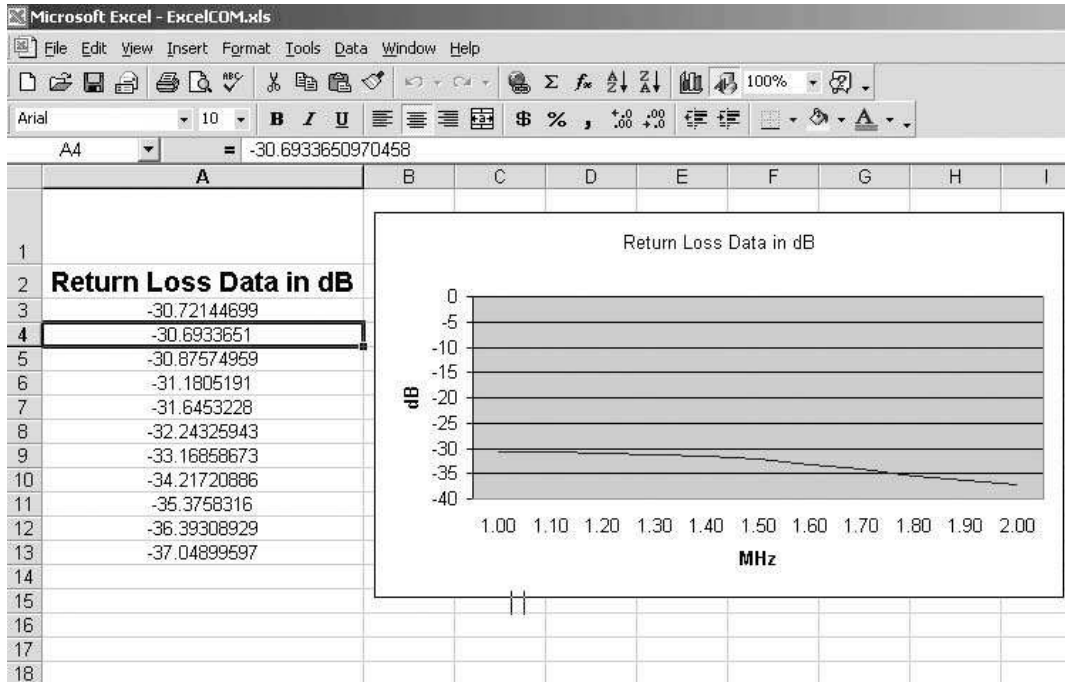

Microsoft Visual C++ Example

Microsoft Visual C++ Configuration

Microsoft Visual C++ version 6 was used for this example. In order to perform this example, create a new project in Microsoft Visual C++. Add a C++ file to the project and paste the following code into the file. The path for the type library in the code below should be changed to reference its location on the development PC.

Microsoft Visual C++ Code

The application can be run on a PC or on the PNA.

```
#include <stdio.h>
#include "atlbase.h"
#include "objbase.h"
// import the PNA type library
//-----
#import "C:\Program Files\Common Files\Keysight\PNA\835x.tlb"
no_namespace, named_guids
int main(int argc, char* argv[])
{
    // interface pointers to retrieve COM interfaces
    IUnknown* pUnk = 0;
    IApplication* pNA = 0;
    IChannel* pChan = 0;
    IMeasurement* pMeas = 0;
    IArrayTransfer* pTrans = 0;
    int i, num_points = 0;
    float* pScalarData;
    HRESULT hr;
    // Initialize the COM subsystem
    CoInitialize(NULL);
    CoInitializeSecurity( NULL, //security descriptor
        0, // authn svc entries
        NULL, // authn svcs
        NULL, // reserved
        RPC_C_AUTHN_LEVEL_NONE,
        RPC_C_IMP_LEVEL_ANONYMOUS,
        0, // authn info
        0, // capabilities
        0); // reserved
    // Create an instance of the network analyzer
    // Request the NA's IUnknown interface
    hr = CoCreateInstance(CLSID_Application,0,CLSCTX_ALL,
        IID_IUnknown, (void**) &pUnk);
    if (!FAILED(hr))
    {
        // QueryInterface for the INetworkAnalyzer interface of the
        NetworkAnalyzer object
        hr = pUnk->QueryInterface(IID_IApplication,(void**)&pNA);
        if (!FAILED(hr))
        {
            // Reset the analyzer to instrument preset
            pNA->Reset();
            // Create S11 measurement
            pNA->CreateSParameter(1,1,1,1);
        }
    }
}
```

Microsoft Visual C++ Code (continued)


```

// Set pChan variable to point to the active channel
pNA->get _ActiveChannel(&pChan);
if (pChan)
{
// Set pMeas variable to point to the active measurement
pNA->get _ActiveMeasurement(&pMeas);
if(pMeas)
{
// Setup the channel for a single trigger
pChan->Hold(true);
pNA->TriggerSignal = naTriggerManual;
pChan->TriggerMode = naTriggerModeMeasurement;
// Make the PNA application visible
pNA->put _Visible(true);
// Set channel parameters
pChan->NumberOfPoints = 11;
pChan->StartFrequency = 1e9;
pChan->StopFrequency = 2e9;
// Send a manual trigger to initiate a single sweep
pChan->Single(true);
// QueryInterface for the IArrayTransfer interface of the
NetworkAnalyzer object
hr = pMeas >QueryInterface(IID _IArrayTransfer,
(void**)&pTrans);
if (!FAILED(hr))
{
// Store the data in the "result" variable
num _points = pChan->NumberOfPoints;
pScalarData = new float[num _points];
pTrans->getScalar(naRawData, naDataFormat _LogMag,
(long *)&num _points, pScalarData);
// Display the result
printf("S11(dB) - Visual C++ COM Example for PNA\n\n");
for (i = 0; i < num _points; i++)
printf("%f\n",pScalarData[i]);
}
}
}
pUnk->Release();
pMeas->Release();
pChan->Release();
pTrans->Release();
pNA->Release();
}
else
{
printf("Programmed failed to connect to the PNA.");
}
}
CoUninitialize();
return 0;
}

```

Microsoft Visual C++ Output

The figure below shows the displayed results when the application is executed.

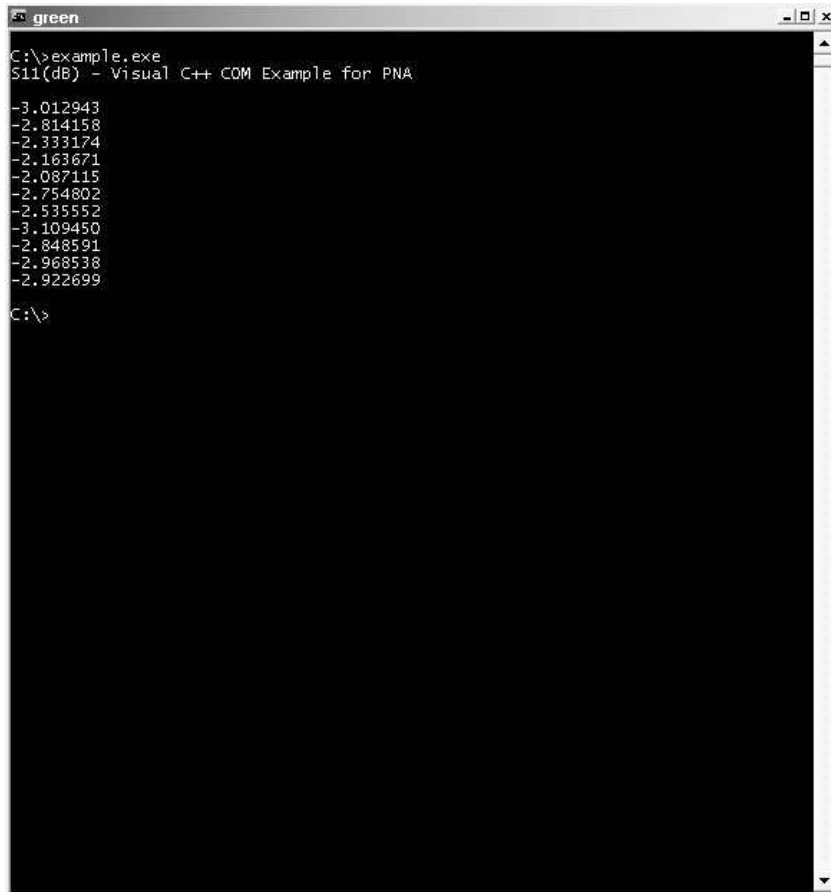


```
green
C:\>example.exe
S11(dB) - Visual C++ COM Example for PNA
-3.012943
-2.814158
-2.333174
-2.163671
-2.087115
-2.754802
-2.535552
-3.109450
-2.848591
-2.968538
-2.922699
C:\>
```


Keysight VEE Example

Keysight VEE Configuration

For this example use Keysight VEE version 6.0 or above which contains the Variant data type used to transfer data from the PNA. The type library for the PNA should be referenced in the Keysight VEE development environment (select **Device > ActiveX Automation References...** in the Vee IDE). The following figure illustrates the reference.

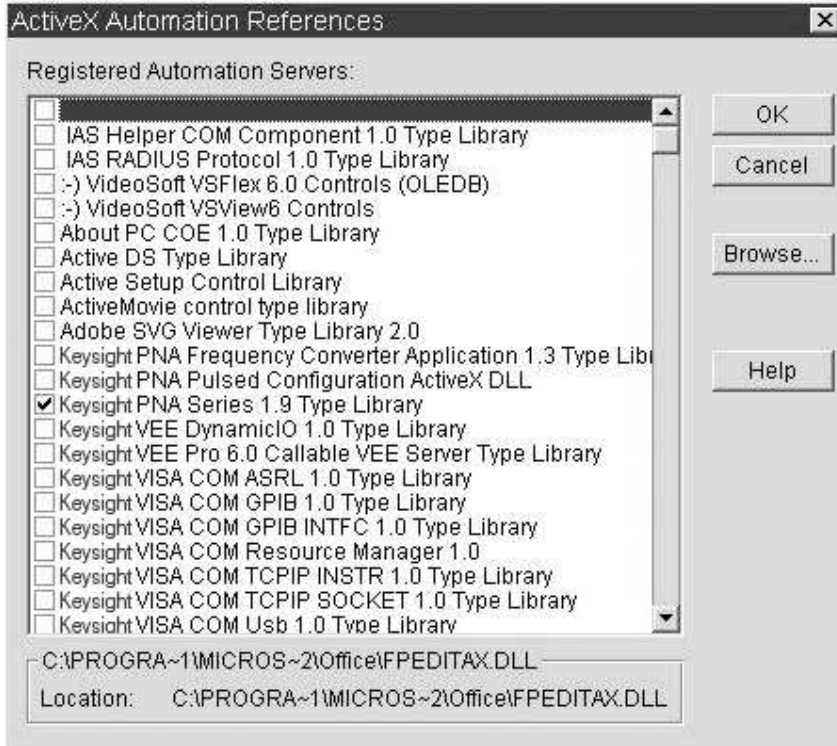

Using the Keysight VEE Object Browser (select **Device > Function & Object Browser**) the developer can see what classes and methods are available for development of applications for the PNA Series analyzer (see figure below).

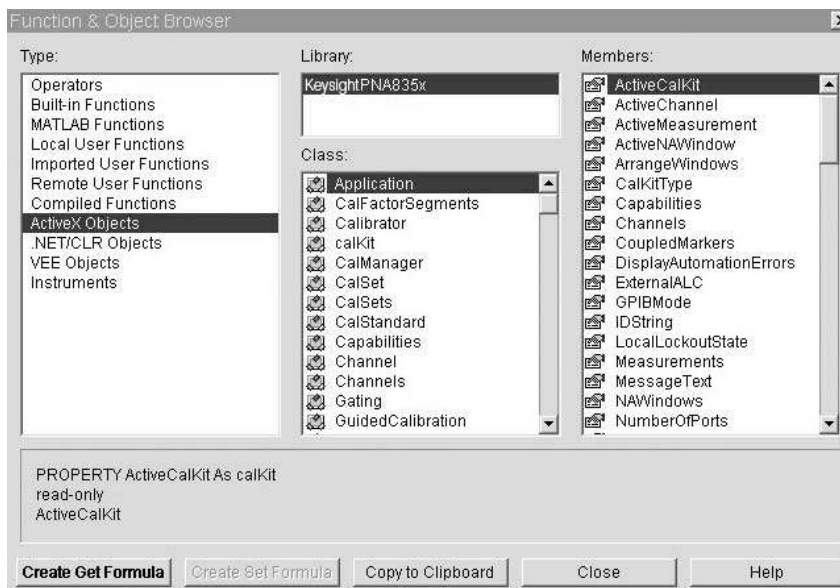

Keysight Vee Code

Keysight VEE version 6.0 or higher must be installed to run the application in this example. There is a runtime version of Keysight VEE that may be used if the application has been saved as "runtime." A free trial version of Keysight VEE can be found on the following web site: <http://www.keysight.com/find/vee/>

The application may be run on a PC or on the PNA Series analyzer. The following screenshot shows the example program.

The screenshot displays the Keysight VEE Pro software interface. The main workspace shows a flowchart with the following steps:

- Start**
- Connect to PNA**: `set app = CreateObject("KeysightPNA835x.Application", "keysight-kppfmj5"); app.reset();`
- Create S11 measurement and set channel and measurement variables**: `app.CreateMeasurement(1, "S11", 1); set chan=app.ActiveChannel; set meas=app.ActiveMeasurement;`
- Setup the channel for a single trigger**: `chan.hold(True); app.TriggerSignal=naTriggerManual; chan.Triggermode=naTriggermodeMeasurement; app.visible=True;`
- Set PNA application parameters**: `chan.numberofpoints=11; chan.startfrequency=(1e9); chan.stopfrequency=(2e9);`
- Send a manual trigger to initiate a single sweep**: `chan.Single(True); data=meas.getData(naCorrectedData, naDataFormat_LogMag);`
- Set PNA application parameters**: `app.quit();`


On the right side, three property windows are visible:

- Declare app**: Name: app, Library: KeysightPNA835x, Scope: Global, Class: Application, Type: Object, Events: Enabled, Sub Type: COM.
- Declare chan**: Name: chan, Library: KeysightPNA835x, Scope: Global, Class: Channel, Type: Object, Events: Enabled, Sub Type: COM.
- Declare meas**: Name: meas, Library: KeysightPNA835x, Scope: Global, Class: Measurement, Type: Object, Events: Not Enabled, Sub Type: COM.

The flowchart also includes a data object labeled "data" and a window titled "S11 (dB) - Keysight VEE COM Example for PNA".

Keysight Vee Output

The figure below shows the displayed results when the application is executed.

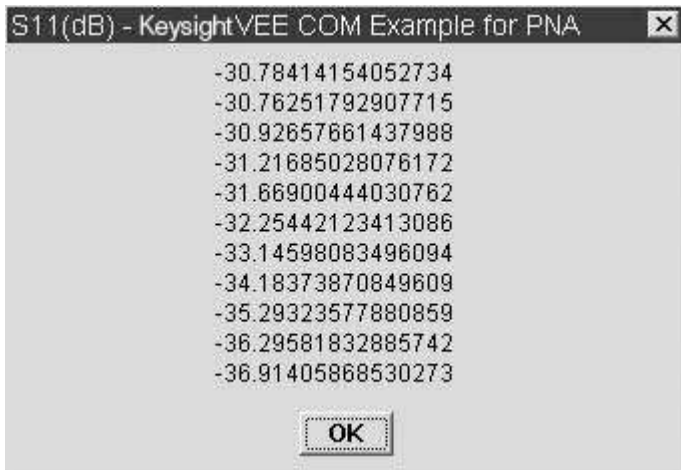

National Instruments LabVIEW™ Example


LabVIEW Configuration

Use National Instruments LabVIEW version 5.0 or above for this example. See the National Instruments LabVIEW documentation or online help for information on using ActiveX objects in the the LabVIEW development environment.

LabVIEW Code


National Instruments LabVIEW 5.0 or higher must be installed to run the application. The application can be run on a PC or on the PNA Series analyzer. The screenshot below was taken from LabVIEW 7.0.

Enter analyzer name here (or leave blank for default)

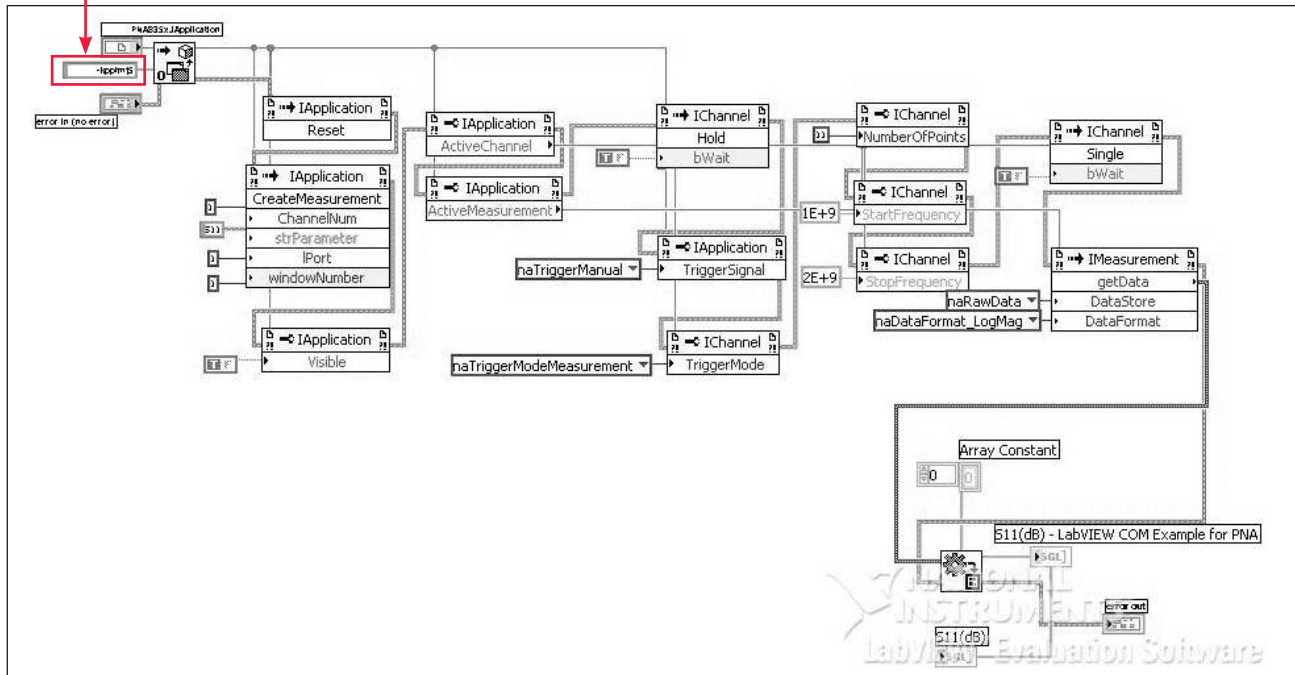

LabVIEW Output

The figure below shows the displayed results when the application is executed. Again, this screenshot was taken from LabVIEW 7.0.

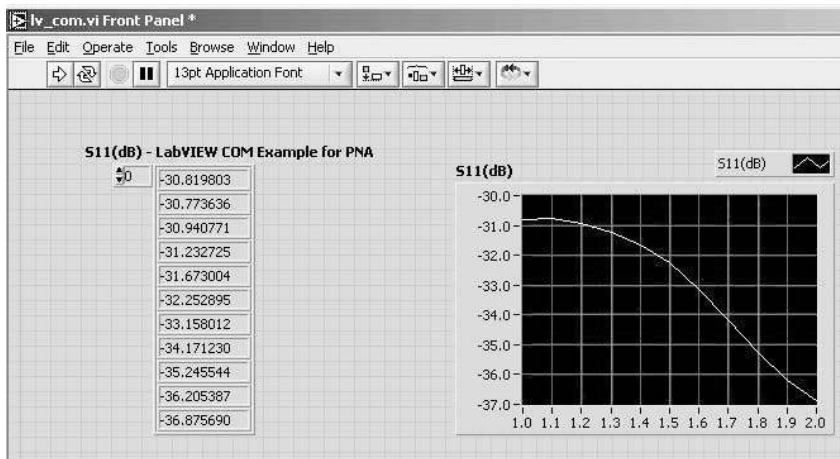

Appendix A: Quick Reference Guide

This section is intended to be used as a quick reference for the steps necessary to register a user on the PNA, share drives between a PC and the PNA, and to configure COM/DCOM. This is just a repeat—in abbreviated form—of information that is contained in more detail in Basic Administration beginning on page 5, and in “Configuring COM/DCOM” beginning on page 11. Please refer back to these sections if you need more detailed information.

Register a User on the PNA

1. Log on to the PNA as administrator.
2. Right-click **My Computer** > Manage.
3. **Local Users and Groups** > right-click **Users** > **New User**
4. Enter **User name** and **Password/Confirm Password** (use PC login and password).
5. **Create** > **Close**

Share Drives

On the PNA:

1. **My Computer** > right-click Local Disk(C:) > **Sharing** > **Share this folder**
2. Optional: Change Share name if desired.

On the PC:

1. Right-click My Computer > Map Network Drive
2. Select **Drive**, enter path (syntax: \\computername\sharename, i.e. \\keysight-kppfmj5\c\$) in **Folder** > **Finish**.

Configure COM/DCOM

Grant User Access (Windows XP)

Please read the note on page 12 to determine whether or not you want to perform this procedure.

On the PNA:

1. Minimize the PNA application, and click **Start > Run > dcomcnfg > OK**
2. Open the following folder sequence:
 - Component Services Window**
 - Component Services**
 - Computers**
 - My Computer**
 - DCOM Config**
3. Right-click **Keysight PNA Series > Properties**
4. Select **Security** tab > **Customize** (under Access Permissions) > **Edit...**
5. Select **Everyone > Remove**, then click **Add** and type a group name or user account name
6. Click **Customize** (under Launch Permissions) > **Edit...**
7. Select **Everyone > Remove**, then click **Add** and type a group name or user account name

Grant User Access (Windows 2000)

Please read the note on page 12 to determine whether or not you want to perform this procedure.

On the PNA:

1. Minimize the PNA application, and click **Start > Run > dcomcnfg > OK**
2. On Applications tab, select **Keysight PNA Series > Properties...**
3. Select **Security** tab > **Use custom access permissions > Edit...**
4. In **Registry Value Permission**, select **Everyone > Remove**, then click **Add** and select one or more groups or users.
5. Click **Add > OK**

Configure the PC for DCOM Access

On the PC:

1. Close any applications that are running.
2. Copy **Program Files\Keysight\Network Analyzer\Automation\pnaproxy.exe** from the PNA to a convenient place on your PC.
3. Run **pnaproxy.exe**

Appendix B: PNA and PNA-L Models

The procedures in this document apply to the following list of the Keysight Technologies, Inc. analyzers. Note that the procedures herein may apply to newer analyzers that had not yet been introduced at the time this document was created.

E8356A
E8357A
E8358A
N3381A
N3382A
N3383A
E8801A
E8802A
E8803A
E8362A/B
E8363A/B
E8364A/B
N5230A
N5250A

Web Resources

Visit our web sites for additional product information and literature.

PNA microwave network analyzers:

www.keysight.com/find/pna

Electronic calibration (ECal):

www.keysight.com/find/ecal

Test and measurement accessories:

www.keysight.com/find/accessories

myKeysight

myKeysight

www.keysight.com/find/mykeysight

A personalized view into the information most relevant to you.



www.axiestandard.org

AdvancedTCA® Extensions for Instrumentation and Test (AXIe) is an open standard that extends the AdvancedTCA for general purpose and semiconductor test. Keysight is a founding member of the AXIe consortium. ATCA®, AdvancedTCA®, and the ATCA logo are registered US trademarks of the PCI Industrial Computer Manufacturers Group.



www.lxistandard.org

LAN eXtensions for Instruments puts the power of Ethernet and the Web inside your test systems. Keysight is a founding member of the LXI consortium.



www.pxisa.org

PCI eXtensions for Instrumentation (PXI) modular instrumentation delivers a rugged, PC-based high-performance measurement and automation system.



Three-Year Warranty

www.keysight.com/find/ThreeYearWarranty

Keysight's commitment to superior product quality and lower total cost of ownership. The only test and measurement company with three-year warranty standard on all instruments, worldwide.



Keysight Assurance Plans

www.keysight.com/find/AssurancePlans

Up to five years of protection and no budgetary surprises to ensure your instruments are operating to specification so you can rely on accurate measurements.



www.keysight.com/go/quality

Keysight Technologies, Inc.
DEKRA Certified ISO 9001:2008
Quality Management System

Keysight Channel Partners

www.keysight.com/find/channelpartners

Get the best of both worlds: Keysight's measurement expertise and product breadth, combined with channel partner convenience.

Windows, Microsoft, NT, 2000, and XP are U.S. registered trademarks of Microsoft Corporation.

Formerly published as Application Note 1408-13

For more information on Keysight Technologies' products, applications or services, please contact your local Keysight office. The complete list is available at: www.keysight.com/find/contactus

Americas

| | |
|---------------|------------------|
| Canada | (877) 894 4414 |
| Brazil | 55 11 3351 7010 |
| Mexico | 001 800 254 2440 |
| United States | (800) 829 4444 |

Asia Pacific

| | |
|--------------------|----------------|
| Australia | 1 800 629 485 |
| China | 800 810 0189 |
| Hong Kong | 800 938 693 |
| India | 1 800 112 929 |
| Japan | 0120 (421) 345 |
| Korea | 080 769 0800 |
| Malaysia | 1 800 888 848 |
| Singapore | 1 800 375 8100 |
| Taiwan | 0800 047 866 |
| Other AP Countries | (65) 6375 8100 |

Europe & Middle East

| | |
|----------------|---------------|
| Austria | 0800 001122 |
| Belgium | 0800 58580 |
| Finland | 0800 523252 |
| France | 0805 980333 |
| Germany | 0800 6270999 |
| Ireland | 1800 832700 |
| Israel | 1 809 343051 |
| Italy | 800 599100 |
| Luxembourg | +32 800 58580 |
| Netherlands | 0800 0233200 |
| Russia | 8800 5009286 |
| Spain | 800 000154 |
| Sweden | 0200 882255 |
| Switzerland | 0800 805353 |
| | Opt. 1 (DE) |
| | Opt. 2 (FR) |
| | Opt. 3 (IT) |
| United Kingdom | 0800 0260637 |

For other unlisted countries:
www.keysight.com/find/contactus
(BP-09-23-14)

