

Keysight Technologies

Measuring Battery Life on Battery-Powered Medical Devices

Application Note



Unlocking Measurement Insights

Integration of modern connectivity technology into patient care continues to grow as more and more healthcare and medical device are connected one way or another. In the new age of Internet of Medical Things (IoMT), various battery-powered wireless medical devices have become increasingly prevalent in our daily lives. Examples of traditional and emerging classes of medical devices include fitness band or smart watch (includes pulse monitor or heartbeat monitor capabilities), blood pressure monitor, pacemaker, pulse oximeter, glucose monitor, thermometer, hearing aids, and others in prototype or ready for introduction before year's end.

These classes of medical devices have common traits - low power, battery-operated, small form factor, mobile, lightweight, and support wireless connection. Depending on the severity of insufficient battery life in these devices, the consequences can range from inconvenience to life-threatening situations.

Therefore, the understanding of the power consumption patterns and battery life requirements of a medical device is the main consideration for all aspect of the electronic consumer medical device design to meet the demanding needs of the end users.

Considerations for Battery Run-Down Test

Battery run-time is determined by battery run-down test. To perform this test, measure the time taken to deplete a fully charged battery or in other words until the battery stops working. The measured time will be the battery run-time. However, this is easier said than done as there are many aspects in this test that every design engineer needs to take into consideration.

Here are the top 4 considerations for battery run-down test:

Consideration 1: Inconsistencies in battery life

Inconsistencies in the battery life between different batteries is common even though they are from the same manufacturer. This is because the batteries may come from different manufacturing batch or factory site.

Recommendation:

Perform the run-down test a couple of times with different batteries.

Consideration 2: Battery's charging condition

It is highly recommended that a fully charged battery is used when performing the test. If the battery is old or partially charged, it will affect the run-time results.

Recommendation:

Ensure that the battery is fully charged and condition the battery by using a battery cycler to cycle the charging of the battery from fully discharged to fully charged.

Consideration 3: Medical device use case

Different modes of the device will draw different amount of current for consumption.

Recommendation:

Set the use case test parameters on a device as the constant variable. Hence during the run-down test, the variable is constant across each test.

Consideration 4: Determine when a device stops working or the battery is fully discharged

Some devices have a low battery LED indication to signal that the battery power is low. However, devices such as pacemakers do not have any low battery indicator.

Recommendation:

Measure the battery voltage when it reaches a certain low voltage threshold and use that as the indicator of when the device stops working.

Power Supply as Battery Simulation

Some design engineers may use a power supply to simulate the battery for the run-down test. However, this method is not accurate or practical as it will introduce more errors and variables to the overall testing. Using a power supply is also not a suitable method as it will never run down like a battery.

However, a power supply with specialized features such as controllable output resistance and excellent transient response on current pulses down can be used to emulate the battery. This approach is very complicated as the power supply's output voltage needs to drop off as the charge is pulled from the power supply into the medical device during the run-down test. The simulation data collection process will be time consuming and the results will be questionable as they may not match with the results obtained using a battery.

Hence, until a more realistic simulation approach is available, a run-down test using batteries is still the preferred method.

More than Run-Time

When designing a device, a design engineer will want to view more and obtain more insight into what is happening during the run-down test. By plotting a voltage and current versus time graph, a much clearer picture of the battery run-down can be achieved.

In order to measure the voltage and current flowing through the battery and the medical device, the tester normally needs the following:


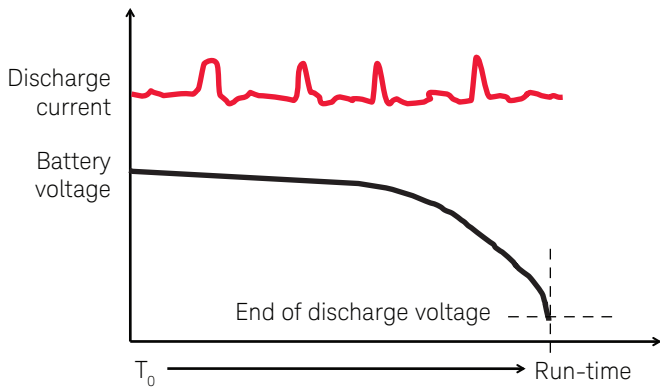


Figure 1. Battery run-down test results

- 2 Digital multimeters (DMMs)
- 2-channel data logger or 2-channel digitizer
- Oscilloscope

Battery voltage measurement is less critical when compared to the current measurement. In order to capture a decaying voltage waveform, a normal DMM or data logger is sufficient for the measurement. However, a current measurement requires a fast digitizer as each device has different current consumption scheme such as sleep mode, standby mode, active mode, and wireless data transmission mode (for wireless device). A device can draw up to hundreds of milliamperes in the active mode, but will only draw microamperes during the sleep mode. High current spikes and transient effects occur when the device is turned on and off frequently. A DMM will not be suitable for capturing the rapid changing current waveform. Additionally, DMM is a burden voltage when it is configured as an ammeter as there is a calibrated current shunt built inside the DMM. This will reduce the voltage at the DUT and burden the overall circuit up to hundreds of millivolts.

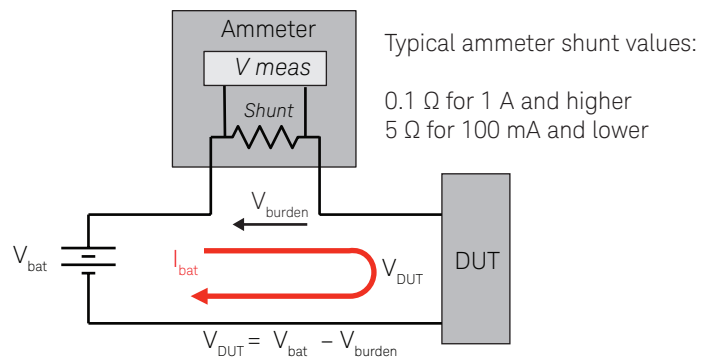

Example calculation of burden voltage of ammeter:

On 100 mA range, 50 mA of I_{bat} yields V_{burden} of 250 mV, so a 4.2 V battery would be reduced to 3.95 V at the DUT.

Figure 2. DMM presents burden voltage when measuring current

Digitizers is the better choice when measuring rapid changing waveform for a long period of time as it has enough bandwidth to capture any rapid changes in the waveform. However, a current shunt is needed as digitizers do not directly measure current. Selecting the right shunt for wide dynamic current measurement that switches from microamperes to amperes is important. If the selected shunt size is for measuring low current, there will be a large voltage drop across the shunt and this will create burden voltage on the circuit. If the selected shunt size is for measuring high current, there will be inaccuracy in low current measurement as there may not be sufficient voltage to pass through the Digitizer. Therefore, a compromise has to be made between burden voltage or low currents inaccuracy when selecting the current shunt size.

Oscilloscope is the best choice to display both the current and voltage measurements waveform as it has good bandwidth for dynamic current measurement and excellent update rate. In addition to that, oscilloscope has a good time correlation with the digital bus and various triggering capabilities to capture the signal accurately. Oscilloscope also faced the same challenge as the digitizer where selecting the right and most suitable current shunt for the measurement is nearly impossible to obtain a good low current measurement and tolerable burden voltage at high current measurement. However, oscilloscope can also be used with high sensitivity current probes which can go down to as low as 50 μ A and with a maximum current range of 5 A. This allows both the large signals and details on fast and wide waveform to be displayed. The limitation on this solution is that it is not able to perform long term measurements.

Solution for Battery Run-Down Test

Keysight Technologies offers the N6781A Battery Drain Analyzer and turnkey software for performing run-down tests for battery powered devices requiring up to 3 A of current. The N6781A can be configured as a zero-burden ammeter. This means that there is zero voltage drop across the instrument as it measures the current flow between the battery and the device. It also offers a unique feature called seamless ranging. This allows instant-and-automatic range change and measure currents from microamperes to amperes at a speed of 100,000 samples per second without losing any data during the range change. The seamless ranging feature makes it ideally suited for measuring dynamic currents during run-down tests. Furthermore, it can also simultaneously measure the voltage across the battery.

With the Keysight 14585 Control and Analysis Software, a battery run-down test can quickly be set up and the run-down measurements can be captured and plotted without coding any software.



Figure 3. Keysight N6781A and N6785A Battery Drain Analyzer is a two-quadrant source and measure unit (SMU) module that plugs into N6705B DC Power Analyzer mainframe and 14585A Control and Analysis Software is a turnkey solution for battery run-down tests on battery powered medical devices



Figure 4. Battery run down test result

Evolving

Our unique combination of hardware, software, support, and people can help you reach your next breakthrough. **We are unlocking the future of technology.**



From Hewlett-Packard to Agilent to Keysight



myKeysight

myKeysight
www.keysight.com/find/mykeysight

A personalized view into the information most relevant to you.

Keysight Infoline

Keysight Infoline

www.keysight.com/find/Infoline

Keysight's insight to best in class information management. Free access to your Keysight equipment company reports and e-library.

KEYSIGHT SERVICES

Keysight Services
www.keysight.com/find/service

Our deep offering in design, test, and measurement services deploys an industry-leading array of people, processes, and tools. The result? We help you implement new technologies and engineer improved processes that lower costs.



Three-Year Warranty

www.keysight.com/find/ThreeYearWarranty

Keysight's committed to superior product quality and lower total cost of ownership. Keysight is the only test and measurement company with three-year warranty standard on all instruments, worldwide. And, we provide a one-year warranty on many accessories, calibration devices, systems and custom products.



Keysight Assurance Plans

www.keysight.com/find/AssurancePlans

Up to ten years of protection and no budgetary surprises to ensure your instruments are operating to specification, so you can rely on accurate measurements.

Keysight Channel Partners

www.keysight.com/find/channelpartners

Get the best of both worlds: Keysight's measurement expertise and product breadth, combined with channel partner convenience.

www.keysight.com/find/medical

For more information on Keysight Technologies' products, applications or services, please contact your local Keysight office. The complete list is available at: www.keysight.com/find/contactus

Americas

Canada	(877) 894 4414
Brazil	55 11 3351 7010
Mexico	001 800 254 2440
United States	(800) 829 4444

Asia Pacific

Australia	1 800 629 485
China	800 810 0189
Hong Kong	800 938 693
India	1 800 11 2626
Japan	0120 (421) 345
Korea	080 769 0800
Malaysia	1 800 888 848
Singapore	1 800 375 8100
Taiwan	0800 047 866
Other AP Countries	(65) 6375 8100

Europe & Middle East

Austria	0800 001122
Belgium	0800 58580
Finland	0800 523252
France	0805 980333
Germany	0800 6270999
Ireland	1800 832700
Israel	1 809 343051
Italy	800 599100
Luxembourg	+32 800 58580
Netherlands	0800 0233200
Russia	8800 5009286
Spain	800 000154
Sweden	0200 882255
Switzerland	0800 805353
	Opt. 1 (DE)
	Opt. 2 (FR)
	Opt. 3 (IT)
United Kingdom	0800 0260637

For other unlisted countries:
www.keysight.com/find/contactus
 (BP-06-08-16)



www.keysight.com/go/quality
 Keysight Technologies, Inc.
 DEKRA Certified ISO 9001:2015
 Quality Management System