

Keysight 16380V Option 001
10 μ F Capacitance Standard
Upgrade Kit

Operation and
Service Manual

Notices

© Keysight Technologies
2001 - 2020

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Keysight Technologies, Inc. as governed by United States and international copyright laws.

Trademark Acknowledgments

Manual Part Number

16380-90111

Edition

Edition 4, February 27, 2020

Printed in Malaysia

Published by:

Keysight Technologies International
Japan G.K,
1-3-3 Higashikawasaki-cho
Chuo-ku
Kobe-shi, Hyogo, Japan

Warranty

THE MATERIAL CONTAINED IN THIS DOCUMENT IS PROVIDED "AS IS," AND IS SUBJECT TO BEING CHANGED, WITHOUT NOTICE, IN FUTURE EDITIONS. FURTHER, TO THE MAXIMUM EXTENT PERMITTED BY APPLICABLE LAW, KEYSIGHT DISCLAIMS ALL WARRANTIES, EITHER EXPRESS OR IMPLIED WITH REGARD TO THIS MANUAL AND ANY INFORMATION CONTAINED HEREIN, INCLUDING BUT NOT LIMITED TO THE IMPLIED WARRANTIES OF MERCHANTABILITY AND FITNESS FOR A PARTICULAR PURPOSE. KEYSIGHT SHALL NOT BE LIABLE FOR ERRORS OR FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH THE FURNISHING, USE, OR PERFORMANCE OF THIS DOCUMENT OR ANY INFORMATION CONTAINED HEREIN. SHOULD KEYSIGHT AND THE USER HAVE A SEPARATE WRITTEN AGREEMENT WITH WARRANTY TERMS COVERING THE MATERIAL IN THIS DOCUMENT THAT CON-

FLICT WITH THESE TERMS, THE WARRANTY TERMS IN THE SEPARATE AGREEMENT WILL CONTROL.

Technology Licenses

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

Declaration of Conformity

Declarations of Conformity for this product and for other Keysight products may be downloaded from the Web. Go to <http://www.keysight.com/go/conformity>. You can then search by product number to find the latest Declaration of Conformity.

U.S. Government Rights

The Software is "commercial computer software," as defined by Federal Acquisition Regulation ("FAR") 2.101. Pursuant to FAR 12.212 and 27.405-3 and Department of Defense FAR Supplement ("DFARS") 227.7202, the U.S. government acquires commercial computer software under the same terms by which the software is customarily provided to the public. Accordingly, Keysight provides the Software to U.S. government customers under its standard commercial license, which is embodied in its End User License Agreement (EULA), a copy of which can be found at <http://www.keysight.com/find/sweula>. The license set forth in the EULA represents the exclusive authority by which the U.S. government may use, modify, distribute, or disclose the Software. The EULA and the license set forth therein, does not require or permit, among other things, that Keysight: (1) Furnish technical information related to commercial computer software or commercial computer software documentation that is not customarily provided to the public; or (2) Relinquish to, or otherwise provide, the government rights in excess of these rights customarily provided to the public to use, modify, reproduce, release, perform, display, or disclose commercial computer software or commercial computer software documentation. No addi-

tional government requirements beyond those set forth in the EULA shall apply, except to the extent that those terms, rights, or licenses are explicitly required from all providers of commercial computer software pursuant to the FAR and the DFARS and are set forth specifically in writing elsewhere in the EULA. Keysight shall be under no obligation to update, revise or otherwise modify the Software. With respect to any technical data as defined by FAR 2.101, pursuant to FAR 12.211 and 27.404.2 and DFARS 227.7102, the U.S. government acquires no greater than Limited Rights as defined in FAR 27.401 or DFARS 227.7103-5 (c), as applicable in any technical data.

Safety Notices

CAUTION

A **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a CAUTION notice until the indicated conditions are fully understood and met.

WARNING

A **WARNING** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a WARNING notice until the indicated conditions are fully understood and met.

- 1. **General Information**
 - Introduction 5
 - The Option 001 Upgrade Kit 5
 - Contents of the 16380V Option 001 5

- 2. **Specifications and Supplemental Performance Characteristics**
 - Specifications for 16388A 7
 - Operating Conditions 7
 - Dimensions 7
 - Weight 7
 - Supplemental Performance Characteristics for 16388A 8
 - Capacitance Temperature Coefficient 8
 - Capacitance Stability 8
 - Maximum Allowable Voltage/Current 8
 - Residual Capacitance 8
 - Storage Conditions 8

- 3. **Service**
 - Calibration 9
 - Recommended Calibration Cycle 9
 - Repair 9

- 4. **Modification of 16380C's Case**
 - Introduction 11
 - Modification Procedure 11

Contents

1 General Information

Introduction

This chapter lists the contents of the kit.

The Option 001 Upgrade Kit

The purpose of the kit is to add one precision capacitor 10 μF (16388A) to the 16380C which consists of three precision capacitors 0.01 μF (16385A), 0.1 μF (16386A), and 1 μF (16387A).

Contents of the 16380V Option 001

See [Table 1-1](#) for the kit contents. If anything is missing, contact the nearest Keysight Technologies office.

Table 1-1

Contents of the 16380V Option 001 Upgrade Kit

Description	Keysight PN	Qty.
16388A (10 μF)	Not Assigned	1
Pad ¹	16380-25001	1
Label	7120-0381	1
Calibration Report	Not Assigned	1
Upgrade Manual (This Manual)	16380-90111	1

1. For modification of your 16380C's case. See Chapter 4.

General Information
Introduction

2 Specifications and Supplemental Performance Characteristics

Specifications for 16388A

Table 2-1

Model	16388A
Nominal Value ¹	10 μ F
Nominal Accuracy ¹	$\pm 0.05\%$
Dissipation Factor ¹	$\leq 5 \times 10^{-4}$

1. Specified at 1kHz under the following ambient conditions:
Temperature: 23 ± 5 °C

Operating Conditions

Ambient Temperature: 23 ± 5 °C

Relative Humidity: Less than 70% RH

Dimensions

142(W) \times 88(D) \times 112(H) mm

Weight

Approximately 1.7 kg

Supplemental Performance Characteristics for 16388A

Capacitance Temperature Coefficient

-20 to 35 ppm/°C

Capacitance Stability

<50 ppm/year @ 1 kHz, 23±5 °C

Maximum Allowable Voltage/Current

40 V peak (ac+dc)/100 mA rms


Residual Capacitance

Table 2-2

16388A	
C_{HG}^1	<50 pF
C_{LG}^1	<50 pF

1. : See figure below.

Figure 2-1

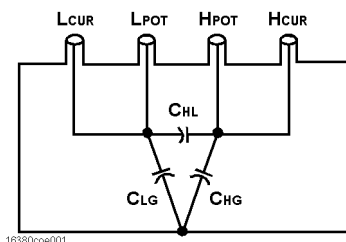

C_{HL} : 4 terminal capacitance

C_{HG} , C_{LG} : Stray capacitance to guard

Storage Conditions

Temperature: -10 °C to +55 °C

Relative Humidity: Less than 85% RH at 40 °C

3 Service

Calibration

Keysight Technologies will calibrate the 16380C together with the 16388A (10 μF). For complete information (price, time required, etc.) on how to have the 16380C and the 16388A (10 μF) calibrated, contact the nearest Keysight Technologies Sales and Service Office. When your 16380C and 16388A (10 μF) requires calibration, all four capacitors should be returned to Keysight Technologies.

Recommended Calibration Cycle

The 16380C and the 16388A (10 μF) should be calibrated at least once a year. More frequent calibration may be required if the capacitors are used in very hot or very cold environments.

Repair

The 16380C and the 16388A (10 μF) contains no replaceable components. If one of the capacitors becomes damaged, or if its capacitance value is outside specified Limits, the capacitor must be replaced. For complete information on service, contact the nearest Keysight Technologies Sales and Service Office.

Service
Repair

4 Modification of 16380C's Case

Introduction


This chapter describes the procedure to modify your 16380C's case for the 16388A (10 μ F).

Modification Procedure

Perform the following steps :


1. Remove a pad of your 16380C's case using a flat-blade screwdriver. See **Figure 4-1** and **Figure 4-2**.

Figure 4-1 Removing the pad (step1)

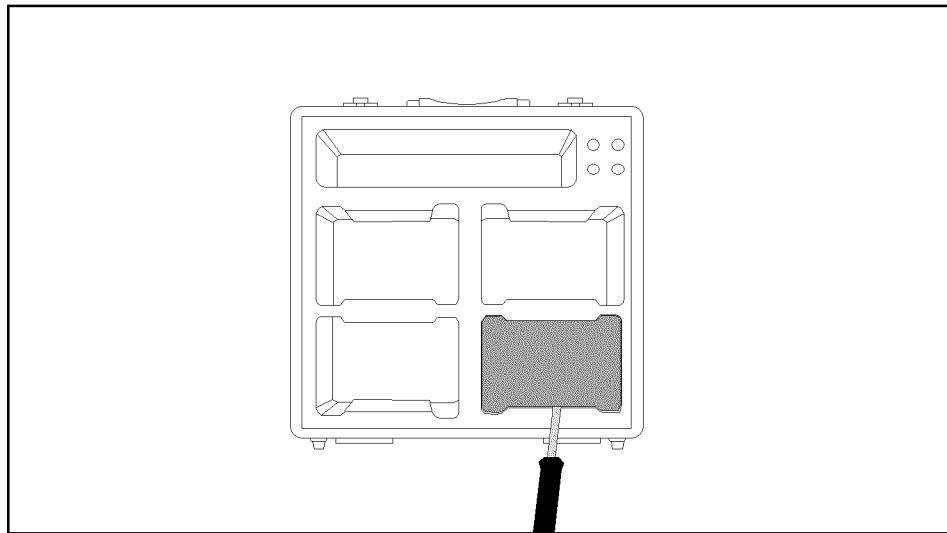


16380coe003

Figure 4-2 Removing the pad (step2)

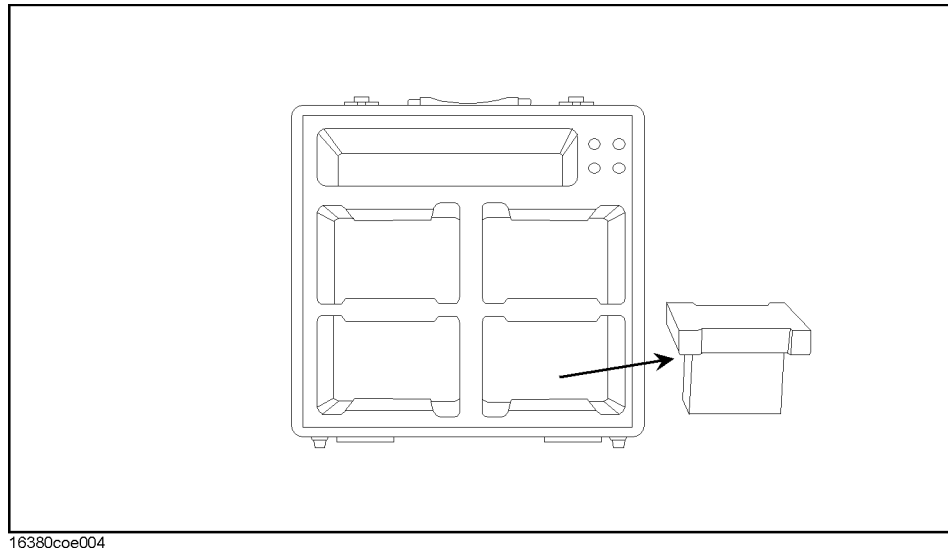

2. Install the Pad (p/n 16380-25001) furnished with this kit in your 16380C's case. See **Figure 4-3**.

Figure 4-3 Installing the Pad (p/n 16380-25001)

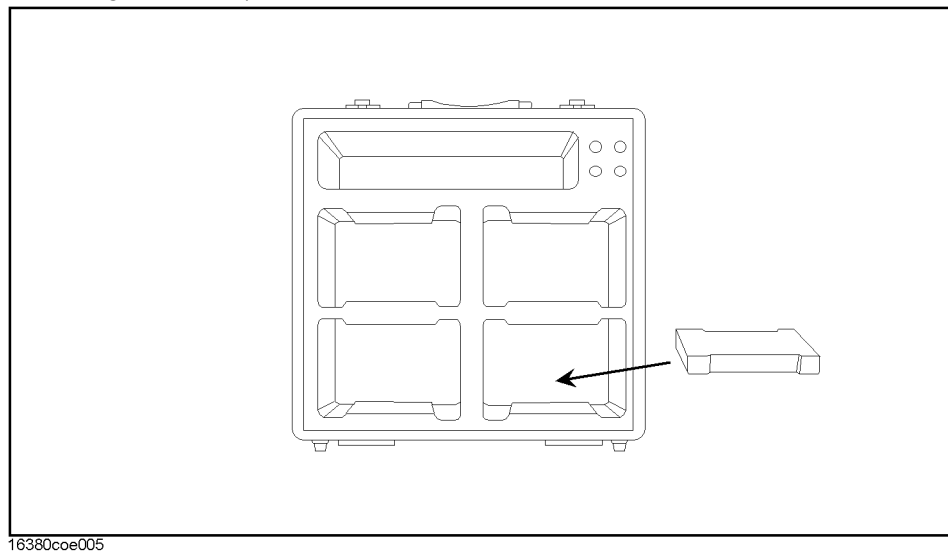

3. Paste a label (p/n 7120-0381) of "OPTION 001" on the position shown in **Figure 4-4**.

Modification of 16380C's Case
Introduction

Figure 4-4 Position of the "OPTION 001" label



Modification of 16380C's Case
Introduction

This information is subject to change without notice.
© Keysight Technologies 2001 - 2020
Edition 4, February 27, 2020



16380-90111
www.keysight.com