

Keysight X-Series Signal Analyzers, Multi-Touch and N9048B PXE EMI Receiver

Option SF2

Security Features, Prohibit Saving Results

Notices

© Copyright 2016 - 2018 Keysight Technologies, Inc.

The information contained in this document is subject to change without notice.

Keysight Technologies makes no warranty of any kind with regard to this material, including but not limited to, the implied warranties of merchantability and fitness for a particular purpose.

Keysight Technologies shall not be liable for errors contained herein or for incidental or consequential damages in connection with the furnishing, performance, or use of this material.

Manual Part Number

N9020-90270

Edition

Edition 1, October 2018

Supersedes February 2016

Printed in USA/Malaysia

Published by:

Keysight Technologies, Inc.

1400 Fountaingrove Parkway

Santa Rosa, CA 95403

Option SF2, Security Features, Prohibit Saving Results

Products Affected:	N9000B CXA Signal Analyzer N9010B EXA Signal Analyzer N9020B MXA Signal Analyzer N9030B PXA Signal Analyzer N9040B UXA Signal Analyzer N9048B PXE EMI Receiver
Serial Numbers:	All
To Be Performed By:	(X) Keysight Service Center (X) Personnel Qualified by Keysight (X) Customer
Estimated Installation Time:	1.0 Hours
Estimated Adjustment and Verification Time:	0 Hours

Introduction

This installation note explains how to install Option SF2 on an X-Series analyzer or PXE EMI receiver. Option SF2 provides changes to the Softkeys and SCPI eliminating the ability to Save or Recall user data. This is at the request of security conscious customers who require no vulnerability in the instrument's UI to save measurement results or user configuration to the instrument's disk drive. For consistency, Recall is eliminated as well. Option SF2 controls access to these Softkeys and SCPI; with Option SF2 the keys & SCPI are locked-out.

Also, the Windows page files are disabled, and this will cause the available memory space for the power-on preloaded applications to decrease.

The option is licensed for one instrument model number/serial number combination. The license file that is downloaded from the web will only install on the designated instrument.

NOTE

1. The latest revision of the X-Series Signal Analyzers software may be downloaded from

http://www.keysight.com/find/xseries_software

If a software update is required, perform the software update BEFORE following the procedure in this document for redeeming and installing the option upgrade license key.

2. This option is licensed for one instrument model/serial number combination. The license key will only install on the designated instrument.

Contents

Quantity	Description	Part Number
1	Installation Note	This note
1	Option Upgrade Entitlement Certificate	5964-5178

Tools Required

- Personal computer with internet access and USB port
- USB storage device with >2GB free memory

Installation Procedure

1. Log out of the default user (instrument) by selecting Start, Log Off.

At the login screen enter:


User name: administrator

Password: Keysight4u!

2. This step disables the paging files. Navigate to C:\Program Files\Agilent\Signal Analysis\Infrastructure and run the SF2RegSetup.reg

A window such as the one shown below will appear. Click on Yes.

Another window will appear notifying you that the SF2RegSetup has been added to the registry. Click OK.

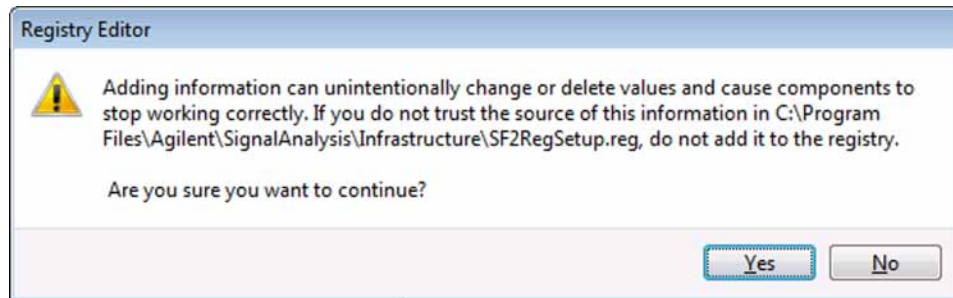

3. On the Windows desktop, click the Configure Applications shortcut. When the window appears click the Deselect All button. Click OK. This step required to assure there will be minimal applications preloaded at power up.
4. Cycle instrument power by turning off the instrument. Since the changes were performed, it may take a bit longer than normal for the instrument to power down.
Power up the instrument and let it boot completely.

License Installation Procedure over USB


1. Locate the Option Upgrade Entitlement Certificate (5964-5178) from the kit.
2. Redeem the Option Upgrade Entitlement Certificate by following the instructions on the Certificate.
3. After redeeming your Option Upgrade Entitlement Certificate you will receive an email with an attached License File.
4. Locate a USB storage device. Perform a virus scan on this device before use.
5. Save the License File to the root directory of the USB Storage Device.
6. Connect the USB Storage Device to the signal analyzer USB port. Windows will detect the new hardware and may display the configuration menu shown in **Figure 1**. This menu may be configured according to your preferences.

Figure 1 USB Storage Device Configuration Menu



7. The signal analyzer will automatically consume the License File. (This may take a few minutes) When the License File is consumed the Keysight License Manager will display a “Successful License Installation” message similar to the one shown in **Figure 2**.

Figure 2 Successful License Installation

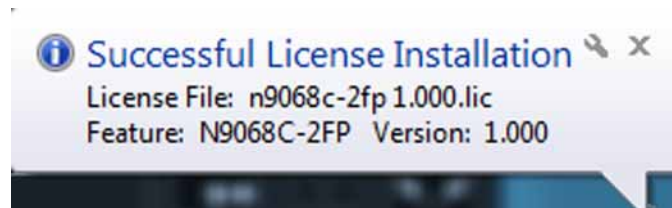

Alternate Installation Procedure

The License File can be manually installed over USB or LAN by placing the license file in the following folder on the signal analyzer

C:\Program Files\Agilent\licensing

Verify the Installation and Instrument Software Version

1. Cycle power on the signal analyzer and wait until the analyzer boots to the measurement application screen.
2. Press **System, Show System** to display a list of installed options.
3. Verify that the installed option list contains N90x0B-SF2 (where "X" is 0, 1, 2, 3, or 4, depending on the model number), or contains N9048B-SF2 for the PXE EMI receiver.
4. Verify that the "Instrument S/W Revision" meets the requirements outlined in the note on [page 4](#) of this document.
5. Press the front panel Save, or Quick Save key. An error message should appear in the message bar at bottom screen that tells you the feature is not available for Option SF2.

Option SF2, Security Features, Prohibit Saving Results

Utilities, Adjustments, and Performance Verification Tests

Utilities Required

None

Adjustments Required

None

Performance Testing Required

None

For assistance, contact your nearest Keysight Technologies Sales and Service Office. To find your local Keysight office access the following URL, or if in the United States, call the following telephone number:

<http://www.keysight.com/find/assist>

1-800-829-4444 (8 am - 8 pm ET, Monday - Friday)



This information is subject to change without notice.

© Keysight Technologies 2016-2018

Edition 1, October 2018

N9020-90270

www.keysight.com